EZEE KLEEN 2.5

Distillation Alternative

User's Guide

Please Read Before Installing & Using this Equipment

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

CONTENTS

FEATURES AND BENEFITS **4**

BEFORE YOU BEGIN

CHECK TO BE SURE YOU HAVE ALL THE FOLLOWING PARTS OR COMPONENTS 5

INSTALLTION OPTIONS

COUNTERTOP INSTALLATION 6

WALL MOUNT INSTALLATION 7

UNDER SINK INSTALLATION 8

PERMANENT MOUNT FAUCET 9

OPTIONAL SEDIMENT CARTRIDGE ..... 10 & 11

OPTIONAL ULTRAVIOLET CARTRIDGE 12

ORGANISMS DESTROYED BY ULTRA VIOLET CARTRIDGE 13

USING AND MAINTAINING YOUR EZEE KLEEN 2.5

PROTOCOL FOR EZEE KLEEN 2.5 14

EXPECTED CARTRIDGE LIFE 15

CHANGING YOUR CARTRIDGES 16

CONNECTING & DISCONNECTING CARTRIDGES 17

MAINTENANCE SUPPLIES 18

INTERNAL COMPONENTS DIAGRAM 19

GUARANTEE/WARRANTY **20**

FZEEKLEEN 2.5
Distillation Alternative

Model: 9000

FEATURES & BENEFITS

QUALITY WATER ONSITE FOR YOUR AUTOCLAVE & CLOSED WATER SYSTEMS QUICKLY AND AFFORDABLY

FEATURES

- Produces 1 gallon (4 litres) of autoclave safe water in two minutes!
- Produces onsite, water of the quality necessary to comply with all autoclave manufactures TDS level guidelines (< 2.5 PPM of dissolved solids)
- Self monitors (unlike bottled water)
- Counter top, wall hung or under counter installation options

APPLICATIONS

- Autoclaves
- Contained dental unit waterline systems

BENEFITS

- Ultra clean water on demand
- Ensure you never run out of water for your autoclave
- Eliminates last minute store runs for water
- Reduce maintenance & equipment failure
- Eliminate bulky storage of bottles
- Consistent water quality < 2.5 PPM
- Ready to use in 5 minutes or installed under counter out of sight
- Save Money

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

BEFORE YOU BEGIN

Install Ezee Kleen 2.5 as per instructions on the mounting option you wish to use.

Page 6: Counter Top Installation (componentry included with unit)

Page 7: Wall Mount Installation (componentry included with unit)

Page 8: Under Counter Installation (requires Optional Kits 9005 & 9007)

Check to be sure you have all the following parts or components:

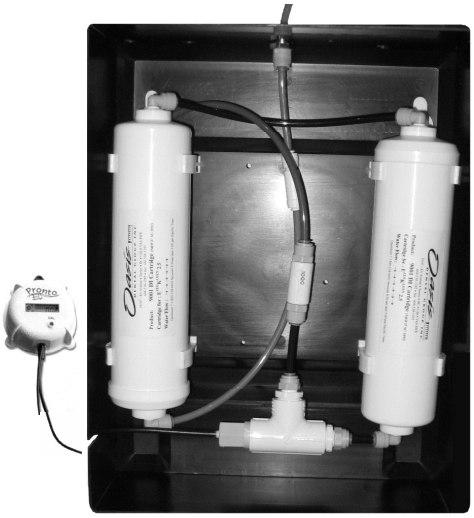

EZEEKLEEN 2.5 Unit
(12"w x 16"h x 6"d)

- Unit
- Cover
- (2) De-ionization cartridges
- Check Valve
- Water Quality Monitor
- Flow Restrictor

Accessories Kit

- 3/8" Short Reach Faucet
- 3/8" Long Reach Faucet
- Diverter Valve
- Tubing
- 1/4" Quick connect elbow

Power Supply

- monitoring system power supply

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

COUNTERTOP INSTALLATION

Using Accessories Kit #9010
(Supplied with unit.)

- Unit Dimensions
  L x H x D
  12 x 16 x 6
- Requires 1 - 110 V electrical receptacles (Monitor)

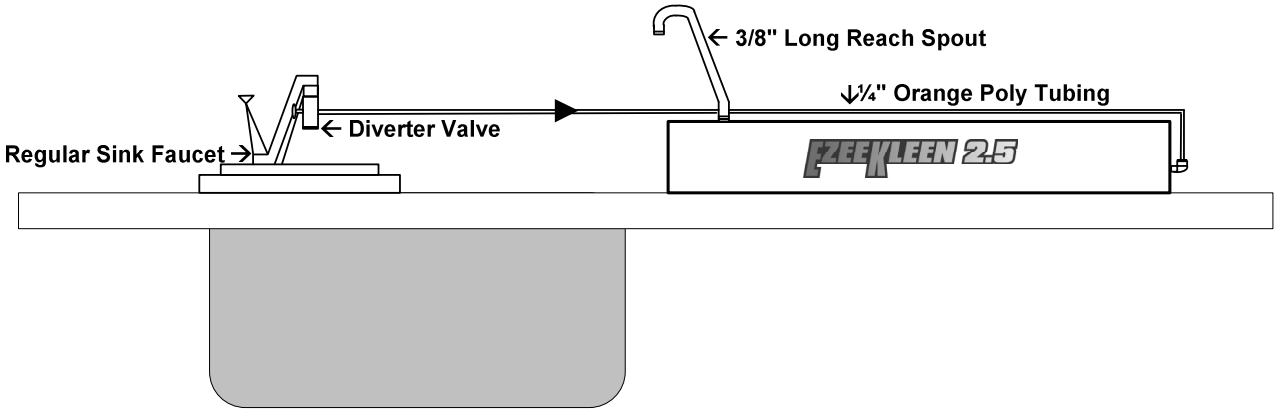

- Place Ezee Kleen 2.5 on counter next to sink
- Remove screen from regular sink faucet
- Attach Diverter Valve to regular faucet (use one of two adapters provided if necessary)
- Insert ¼" quick connect elbow into top of unit
- Insert 3/8" Long Reach Spout into front of unit
- Plug in Monitor Transformer
- Run one cup of water through Unit
- Ensure monitor reading is below 5.00

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

WALL MOUNT INSTALLATION

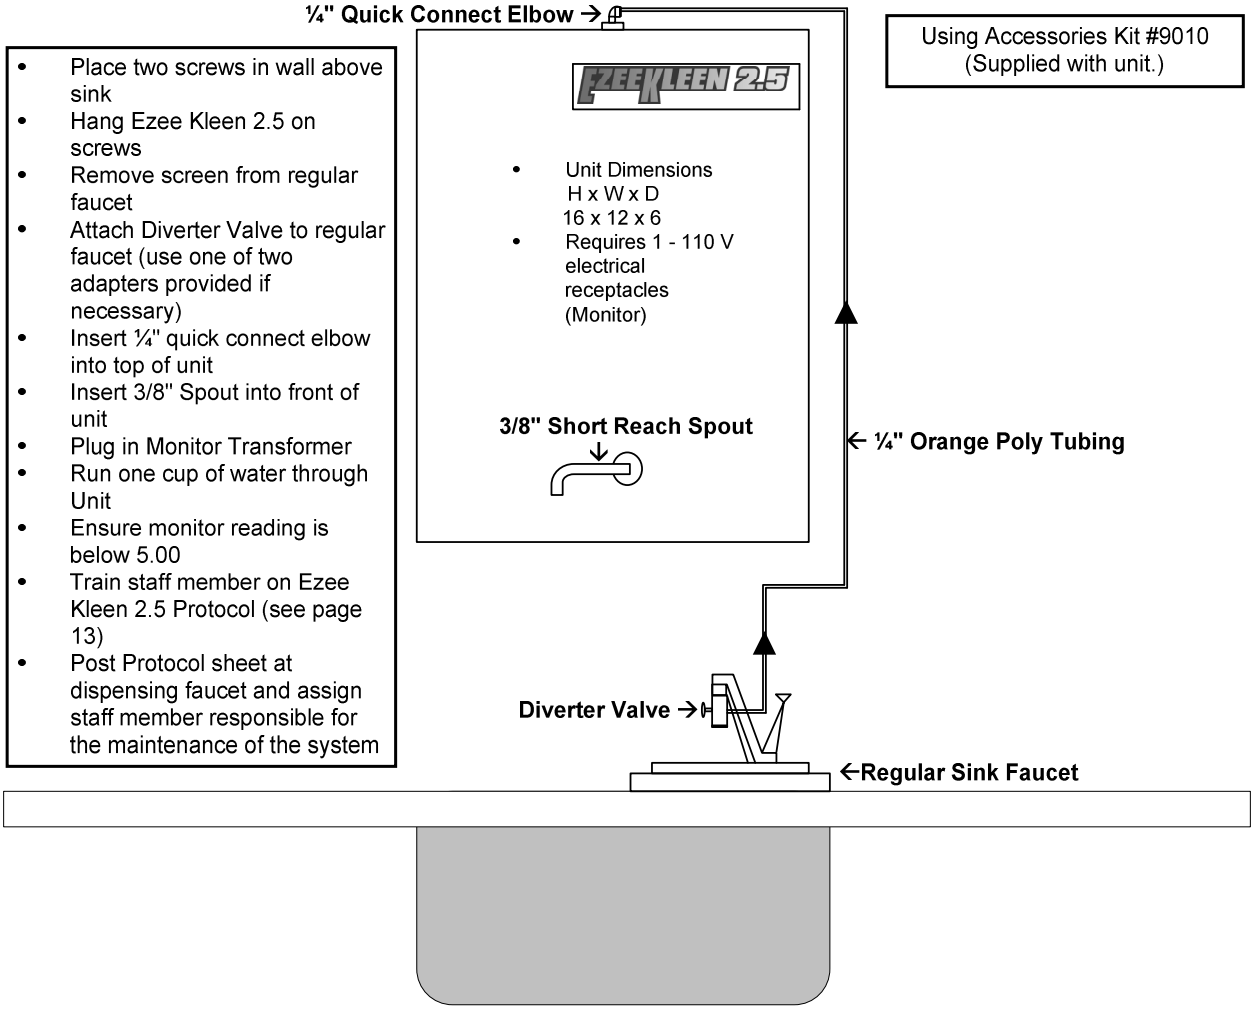

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

UNDER SINK INSTALLATION

Use parts:
#9005 Ezee Kleen 2.5 Hard Plumbing Kit
AND
#9007 Ezee Kleen 2.5 Permanent Mount Faucet

This unit produces Ultra-pure de-mineralized water.
Intended uses: Steam autoclaves, Self contained delivery systems, ultra-sonic baths.

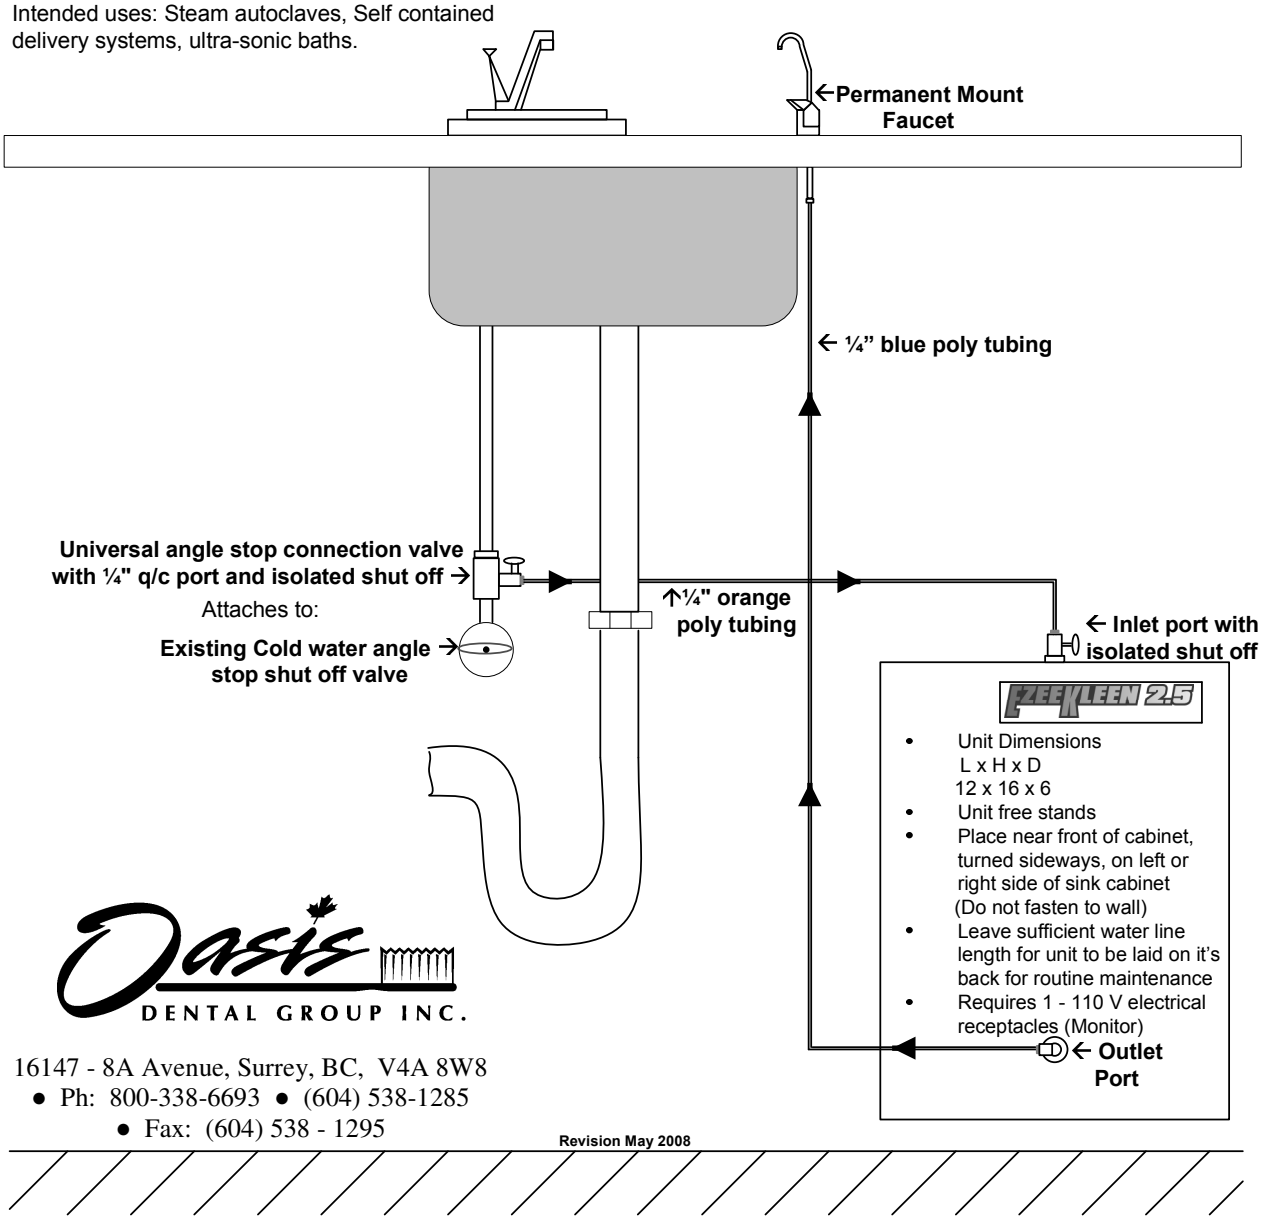

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8
● Ph: 800-338-6693 ● (604) 538-1285
● Fax: (604) 538 - 1295

Revision May 2008

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

9007 PERMANENT MOUNT FAUCET

Use faucet to deliver autoclave safe water from Ezee Kleen 2.5 installed undercounter.
Order kit #9005, Ezee Kleen 2.5 Hard Plumb Kit, to install unit undercounter. Includes all hardware for supply line connection and isolated shut-off valve at supply connection and unit.

ALSO INCLUDES:

- Ferrule
- Plastic Compression Ring
- Compression Nut

Alternative tubing connection option

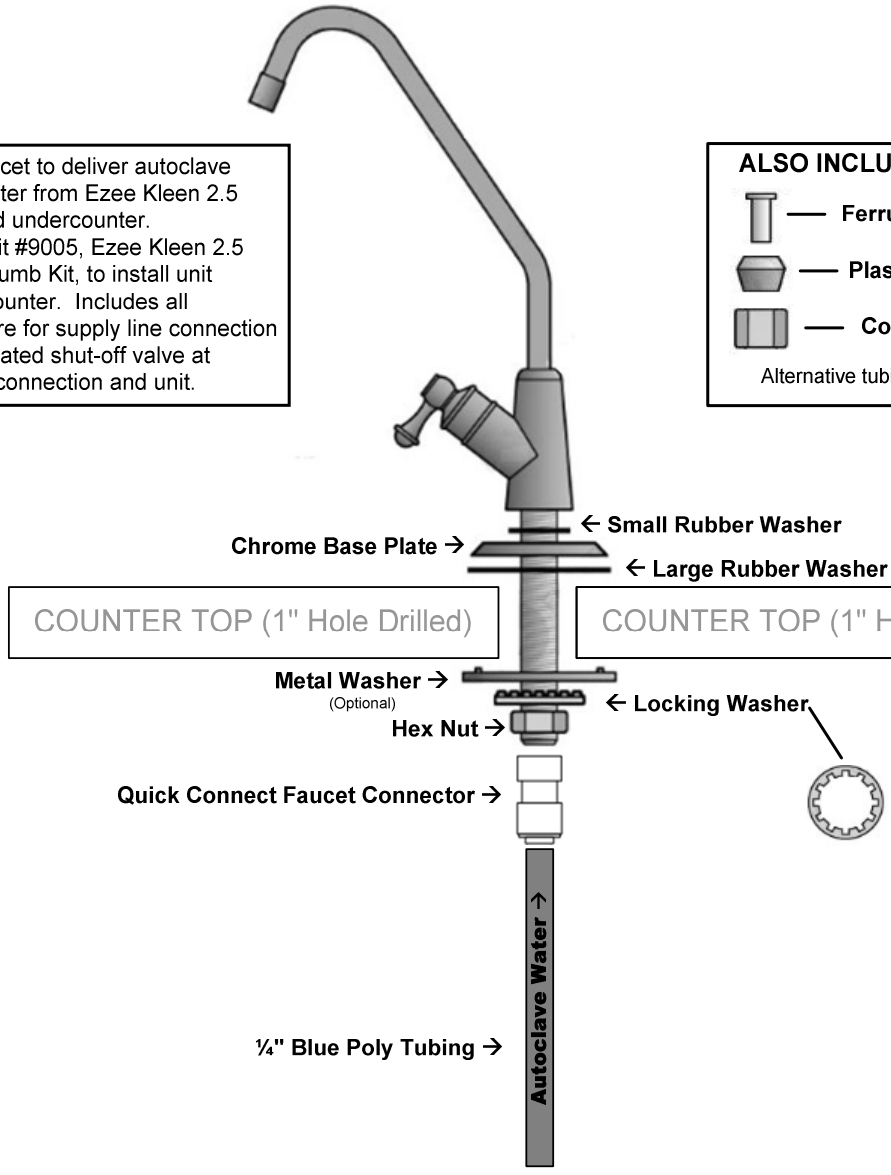

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Optional Sediment Cartridge

Are you Maximizing the Life of your DI Cartridges?

The Ezee Kleen 2.5's 9001 Deionization Cartridges are designed to remove dissolved solids such as iron, calcium, magnesium, sodium, etc.

Public utilities systems are vulnerable to larger particulate matter that can be characterized as sediment/suspended solids. These suspended solids could be sand, silt, flux, metal flaking from older plumbing (eg. Galvanized steel) organic matter, etc.

Sediment/Suspended Solids can reduce the flow rate of the Ezee Kleen 2.5 DI Cartridges and prematurely shorten their life.

Sediment/Suspended Solids enter the utilities water main system from such sources as:

- Water main system flushing programs
- Water main repair or expansion projects
- Water main breaks
- New tie ins for new commercial or residential construction
- Older buildings, especially those still having galvanized piping

Maximize the life of the Ezee Kleen 2.5's 9001 Deionization Cartridges by using our Ezee Kleen 2.5 9002 Sediment Cartridge

- Annual change recommendation

Fast Simple Installation

Use the 9003 Sediment Cartridge Install Kit to install the Sediment Cartridge for the first time. Takes minutes to install.

For less than 10 cents a day!

9002 Sediment Cartridge (change annually)
9003 Sediment Cartridge Install Kit (includes one Sediment Cartridge)

Oasis DENTAL GROUP INC.
16147 - 8A Avenue, Surrey, BC V4A 8W8 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538-1295
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

OPTIONAL SEDIMENT CARTRIDGE

Installing Optional Sediment Cartridge

First time: Order Part #9003 Sediment Install Kit (Includes one cartridge.) Annually: Order Part #9002 Sediment Cartridge

1. Attach brackets to the Ezee Kleen 2.5 Case using Sediment install kit.
2. Move the 9001 DI Cartridge that is on the left to center brackets

Yearly Change out: Snap out and discard old Sediment Cartridge then follow steps 3 & 4

3. Remove protective white dust plugs from either end of the new Sediment Cartridge (see page 16 for quick connect fitting instructions) and snap in the new Sediment Cartridge into left brackets
4. Attach tubing and components as shown in the below diagram
5. Mark Sediment Cartridge for annual change out

Tip: Use Patient scheduler to log reminder to change Ezee Kleen 2.5 Sediment Cartridge in one years time

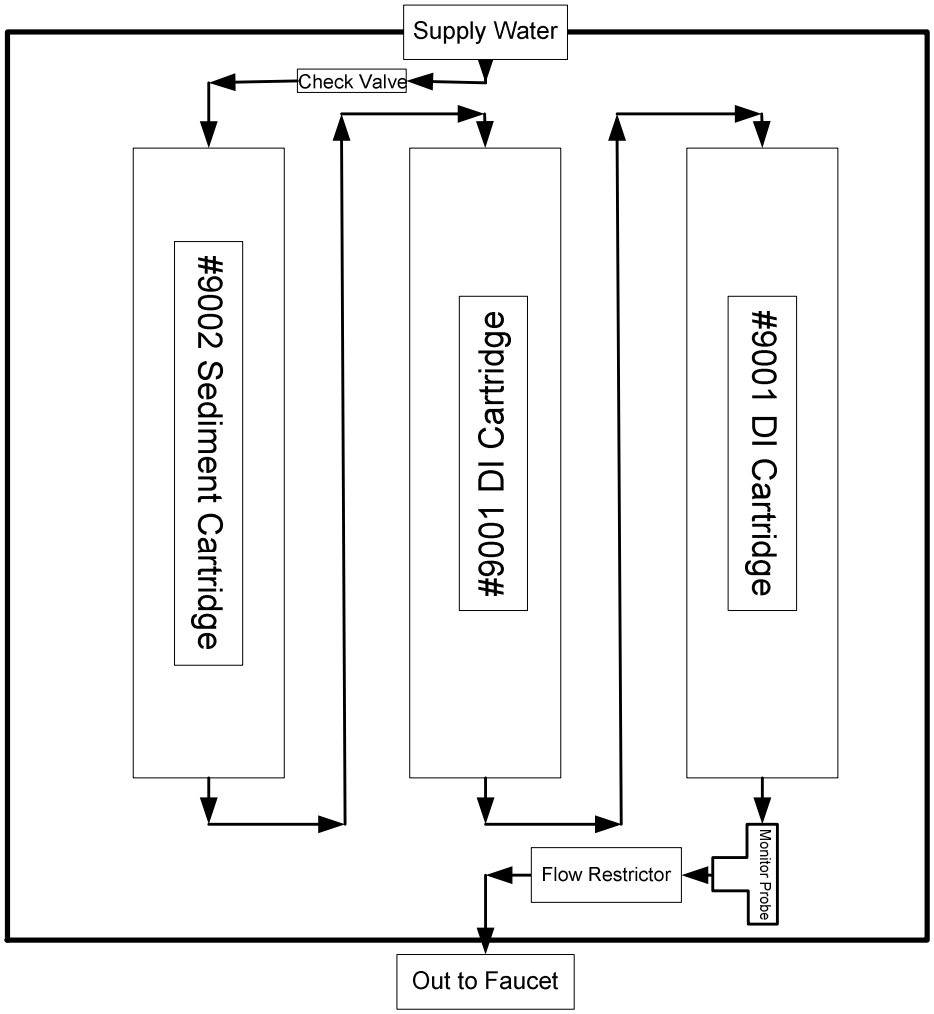

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Optional Ultraviolet Cartridge

Turn your Ezee Kleen 2.5 into an Ultra Pure Water System!

Produce water Ideal for your Self Contained Dental Unit Water Systems

Why Use Ezee Kleen 2.5 Water with our Optional Ultraviolet Cartridge in your Self Contained Dental Unit Water System?

Destroy Microbial Contamination Before it Becomes a Problem!
The Ezee Kleen 2.5 Ultraviolet (UV) Cartridge produces 32,000 w-sec/cm^2 of UV radiation which destroys bacteria, viruses and other micro-organisms by interfering with the DNA and RNA in the organisms' reproductive cycles.
Effective on bacteria, algae, viruses & yeasts.

Reduce the change frequency of micro-filtration cartridges on your dental lines to save time and money.

No organic matter (algae, etc.) ***and inorganic elements*** (dissolved solids - sodium, calcium, etc.) means no food and nutrients for bacteria survival and biofilm development. Slower growth if it does occur.

Reduce chemical treatment frequency on your dental lines to save time, money and deterioration of lines, o-rings, gaskets and equipment from exposure to harsh chemicals.

No Microbes means less chance of biofilm growth in the first place

Additional Benefits of Quality Ezee Kleen 2.5 Water!

Autoclave Water - onsite, on demand - 1 gallon (4 litres) in 2 minutes water of the quality necessary to comply with all autoclave manufacturer's TDS level guidelines

Eliminate the bulky storage of bottles

Ensure you never run out of water for your autoclaves - Eliminate last minute store runs for water.

Self monitor for consistent water quality (Unlike bottled water)

Maximize the efficiency & life of dental unit equipment and instruments. Quality water ensures your equipment does not become clogged with mineral scale that can cause malfunction, increased energy usage and shortened life.

Save Money!!!

Fast Simple Installation

Use the 9004 Ultraviolet Cartridge Install Kit to install the Ultraviolet Cartridge for the first time. Takes only minutes to install. No special tools required.

9004 Ultraviolet Cartridge Install Kit (Includes one lamp)
9004-01 Ultraviolet Replacement Lamp (Change Annually)

Oasis DENTAL GROUP INC.
16147 - 8A Avenue, Surrey, BC V4A 8W8 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538-1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

ORGANISMS DESTROYED BY Ezee Kleen 2.5 ULTRAVIOLET RADIATION CARTRIDGE
GERMICIDAL LEVEL (w-sec/cm^2)

The **EZEEKLEEN 2.5 Ultraviolet Cartridge** effectively uses Ultraviolet (UV) radiation to destroy bacteria, viruses and other microorganisms by interfering with the DNA and RNA in the organisms' reproductive cycles. The contact disinfectant property of UV radiation energy is measured in microwatt-seconds per square centimetre (w-sec/cm^2).
The **EZEEKLEEN 2.5 UV Cartridge** produces 32,000 to 35,000 (w-sec/cm^2).

BACTERIA	
Agrobacterium	8,500
Bacillus anthracis	8,700
Bacillus megaterium (vegetative)	2,500
Bacillus subtilis (vegetative)	11,000
Clostridium tetani	22,000
Corynebacterium diphtheriae	6,500
Escherichia coli	7,000
Legionella bozemanii	3,500
Legionella dumoffii	5,500
Legionella gormanii	4,900
Legionella micdadei	3,100
Legionella longbeachae	2,900
Legionella pneumophila	3,800
Leptospira interrogans (Infectious Jaundice)	6,000
Mycobacterium tuberculosis	10,000
Neisseria catarrhalis	8,500
Proteus vulgaris	6,600
Pseudomonas aeruginosa laboratory strain	3,900
Pseudomonas aeruginosa environmental strain	10,500
Rhodospirillium rubrum	6,200
Salmonella enteritidis	7,600
Salmonella paralyphi (Enteric Fever)	6,100
Salmonella typhimurium	15,200
Salmonella typhosa (Typhoid Fever)	6,000
Sarcinia lutea	26,400
Serratia marcescens	6,200

BACTERIA, continued	
Shigella dysenteriae (Dysentery)	4,200
Shigella flexneri (Dysentery)	3,400
Shigella sonnei	7,000
Staphylococcus epidermidis	5,800
Staphylococcus aureus	7,000
Streptococcus faecalis	10,000
Streptococcus hemolyticus	5,500
Streptococcus lactis	8,800
Viridans streptococci	3,800
Vibrio cholerae	6,500
ALGAE	
Chlorella vulgaris (algae)	22,000
VIRUSES	
Bacteriophage (E.coli)	6,600
Hepatitus virus	8,000
Influenza virus	6,600
Poliovirus (Poliomyelitis)	21,000
Rotavirus	24,000
YEAST	
Baxter's yeast	8,800
Brewer's yeast	6,600
Common cake yeast	13,200
Saccharomyces var. ellipsoideus	13,200
Saccaromyces sp	17,600

EZEEKLEEN 2.5 UV Cartridge
Includes all componentry necessary for initial installation, includes 9001-01
Product ID: 9004
Dimensions: 11.5" x 2.25"/ 29cm x 6 cm
Weight: 1 lb/0.45 kg
Replacement Lamp: 9004-01
Recommended change frequency: 9000 hrs or annually
Power Supply: 55 VAC; 60 Hz; 16 amp. (Optional European format available)
Approved Componentry: UL/CSA approved, made of FDA approved materials and requires no MSDS reporting

These data are believed to be reliable but do not imply any warranty or performance guarantee. Actual performance will vary.
Microbial testing may be appropriate to determine suitability of water for intended use.

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

PROTOCOL FOR USAGE

When drawing water from the Ezee Kleen 2.5 ALWAYS ensure the following protocol is used:

- Tip: Photocopy and laminate this page or contact Oasis Dental Group Inc. Customer Support for a free laminated copy and post at the Ezee Kleen 2.5 dispensing faucet.
- Water is suitable for use in autoclaves, self contained dental unit water systems, ultrasonic baths, instrument cleaning and film developers
- Collect and store Ezee Kleen 2.5 autoclave safe water in clean containers marked "Autoclave Water Only" "No Tap Water" "Keep Lid On" "Store Only 48 Hours".
- Label the Dispensing Faucet "Autoclave Water - Always Check Monitor while Drawing Water".
- Disregard monitor when not dispensing water from the unit (ie. when unit sits idle)
- Check Ezee Kleen 2.5 Monitor each time water is drawn to ensure red light is not flashing and reading is less than 5.00 u/s.
- Regularly inspect the containers for cleanliness.
- When storing filled containers ensure caps remain on.
- Avoid storing or drawing water in an unclean environment.
- Avoid storing the water more than 48 hours.
- Ensure the working area around the dispensing faucet and especially the dispensing faucet itself remains clean.
- Avoid running equipment that has the potential to create dust or particulate matter in the atmosphere when drawing water.
- Use "Patient Scheduler" to schedule maintenance for Ezee Kleen 2.5 annually.
- See page 15 of user's manual for "Changing Your Cartridges"
- Failure to comply with manufacturer's Protocol for Usage" and below maintenance recommendations could result in water not suitable for intended use

Cartridge	**9001 DI Cartridge's (Both Cartridges)**	**9004-01 UV Lamp (Optional) enhances sterility of water**	**9002 Sediment Cartridge (Optional) enhances life of DI Cartridges**
Maintenance	Change when monitor reads > 5.00 with water flowing (red light will begin to flash as secondary indication)	Change Annually	Change Annually
Last Maintained			
Changed by:			
Cartridge Supplier:			
Staff member responsible for maintenance of the Ezee Kleen 2.5:			

Questions? Contact customer support Mon – Fri, PST, 8:00am – 5:00pm.

Oasis DENTAL GROUP INC.
16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

EXPECTED CARTRIDGE LIFE

Oasis Dental Group Inc. is unable to warranty this unit's gallon production of autoclave safe water as the quantity of autoclave safe water produced by a set of DI cartridges is dependent upon the PPM (PARTS PER MILLION) level of TDS (TOTAL DISOLVED SOLIDS) in the supply water to the unit. The unit of measure is sometimes expressed in mg/L which is equivalent to PPM. TDS levels can change significantly for different water utilities.

The Ezee Kleen 2.5 is recommended for offices with tap water Total Dissolved Solids (TDS) under 100 PPM (mg/L). For area's greater than 100 PPM (mg/L) consider our EZEE KLEEN 2.5 HD 4 - Stage Ultra Clean Water System (Model # 8000).

If you are concerned with cartridge life do not use this unit until you have determined TDS levels for your utility and applied it to the below formula.

28,000 ÷ PPM (mg/L) LEVEL OF SUPPLY WATER TDS = LITERS
LITERS ÷ 3.78 USA (or) 4.2 Canada = GALLONS/ one set of DI Cartridges

If gallon production from the Ezee Kleen 2.5 is unacceptable consider our Ezee Kleen 2.5 HD model. By way of advanced technologies the gallon production from the Ezee Kleen 2.5 HD is (10 times) the life of the Ezee Kleen 2.5.

To determine your TDS level for use in the above formula contact Oasis Dental. All Water Utility companies / municipalities supplying water for public consumption are required by municipal, state or provincial regulation to maintain on file a "Water Quality Report" or "Consumer Confidence Report" which reports TDS levels as a secondary parameter. Oasis Dental maintains an extensive library of these "Water Quality Reports" by utility/ municipality and can assist you in determining your TDS level.

NOTE: The above formula calculates expected autoclave safe water production from this unit under optimal working conditions. Gallon production is also affected by the turbidity of supply water to the unit. Turbidity is a measurement of the suspended solids found in municipal water supplies and is represented by organic and inorganic matter such as sand, silt and algae. In areas of high turbidity this unit's performance can be enhanced to optimal levels by the addition of **Oasis Dental Group Inc.'s** optional sediment cartridge. (PART # 9002)

For assistance contact Oasis Dental Group Inc.'s customer support department: 8:30 AM - 5:00 PM PST, Monday - Friday at 1-800-338-6693

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

CHANGING YOUR CARTRIDGES

Tip: Only read monitor when the water is flowing through the Ezee Kleen 2.5

Step one: Obtain shrink wrapped 9001 DI Cartridge two pak. Remove cartridges from the shrink film.

Step two: One at a time remove the white dust plugs from either end of the cartridge, following the quick connect instructions given on page 17 of the users manual. The quick connect feature is on every fitting in the Ezee Kleen 2.5.

Step three: Turn off the supply water to the Ezee Kleen 2.5.

Step four: Disconnect the 90 degree elbows from each end of the 9001 DI Cartridges using the quick connect feature.

Step five: Snap the old 9001 DI Cartridges out of the brackets. Discard the old Cartridges.

Step Six: Snap the new 9001 DI Cartridges into the brackets.

→→→→ ***Arrows on cartridge labels indicate the direction of water flow*** →→→→

Step Seven: Reconnect the 90 degree elbows to each end of the 9001 DI Cartridges.

Step Eight: Turn supply water on to the Ezee Kleen 2.5 and run until there is a steady stream of water. The monitor should read below 5.00 and the red light will stop flashing.

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

CONNECTING & DISCONNECTING CARTRIDGES

The Ezee Kleen 2.5 is equipped with a unique collet locking system that allows cartridge changes to take only seconds and requires no special training or tools.

To make a connection

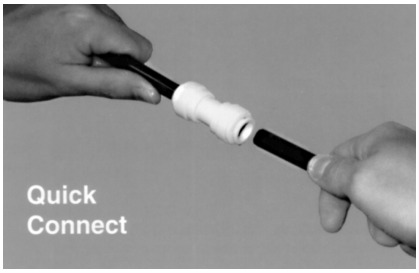

1. Cut tube square

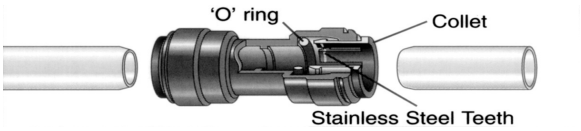

Cut tube square. It is essential that the outside diameter be free of score marks and that burrs and sharp edges be removed before inserting into fitting. For soft thin walled plastic tubing we recommend the use of a tube insert.

2. Insert tube

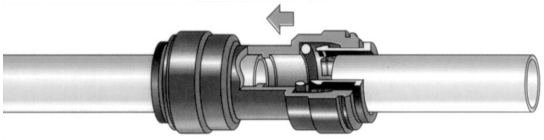

Fitting grips before it seals. Ensure tube is pushed into the tube stop.

3. Push up to tube stop

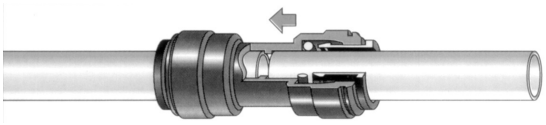

Push the tube into the fitting to the tube stop. The collet (gripper) has stainless steel teeth which hold the tube firmly in position while the 'O' ring provides a permanent leak proof seal.

4. Pull to check secure

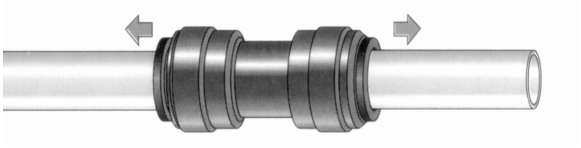

Pull on the tube to check that it is secure. It is a good practice to test the system prior to leaving site and/or before use.

Disconnecting

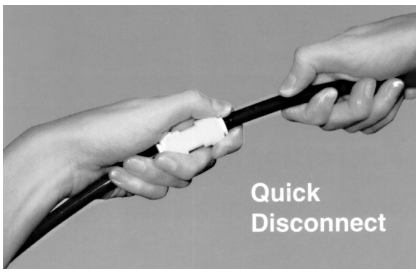

Push in collet and remove tube



To disconnect, ensure the system is depressurized before removing the tube. Push in collet squarely against face of fitting. with the collet held in this position, the tube can be removed. The fitting can then be reused.

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

MAINTENANCE SUPPLIES

TO ORDER YOUR SUPPLIES

1) Contact your authorized **EZEEKLEEN 2.5** dealer.
For easy reference, enter your Dealer's name and contact information here:

_____

_____

_____

Or

2) Contact **Oasis Dental Group** at:
1-800-338-6693 or 1-604-538-1285
Fax: 1-604-538-1295
Mail: 16147 - 8A Avenue, Surrey, BC, CANADA, V4A 8W8
Website: www.oasisdentalgroup.ca
Email: info@oasisdentalgroup.ca

EzeeKleen 2.5 - Complete Unit - # 9000

De-ionization Cartridges - # 9001

- change cartridges when monitor reads > 5.00 µs **with water flowing** (red light will begin to flash as a secondary indication) water is greater than 2.5 PPM (mg/L) of dissolved solids and is unsafe to use in autoclave.

OPTIONAL FEATURES

- **Sediment Cartridge - #9002**
  Change after one year of use.
- **Sediment Install Kit - #9003**
  Order for initial Sediment Cartridge install.
- **Ultra-Violet Cartridge - #9004**
  Order for initial Ultra-Violet Cartridge install.
- **Ultra-Violet Cartridge Replacement Lamp - #9004-1**
  Change after one year of use.
- Under Sink Installation Kit - #9005 (see page. 8)
- Permanent Mount Faucet - #9007 (see page. 9)
- Total Dissolved Solids Tester (Handheld)
- For water testing contact Oasis Dental Group or a local water testing facility.

TIP: Use Patient scheduler to log a reminder to change Sediment Cartridge and Ultra Violet Lamp after one year of use.

Oasis DENTAL GROUP INC.
16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

EZEE KLEEN 2.5
Distillation Alternative

Model: 9000

INTERNAL COMPONENTS DIAGRAM

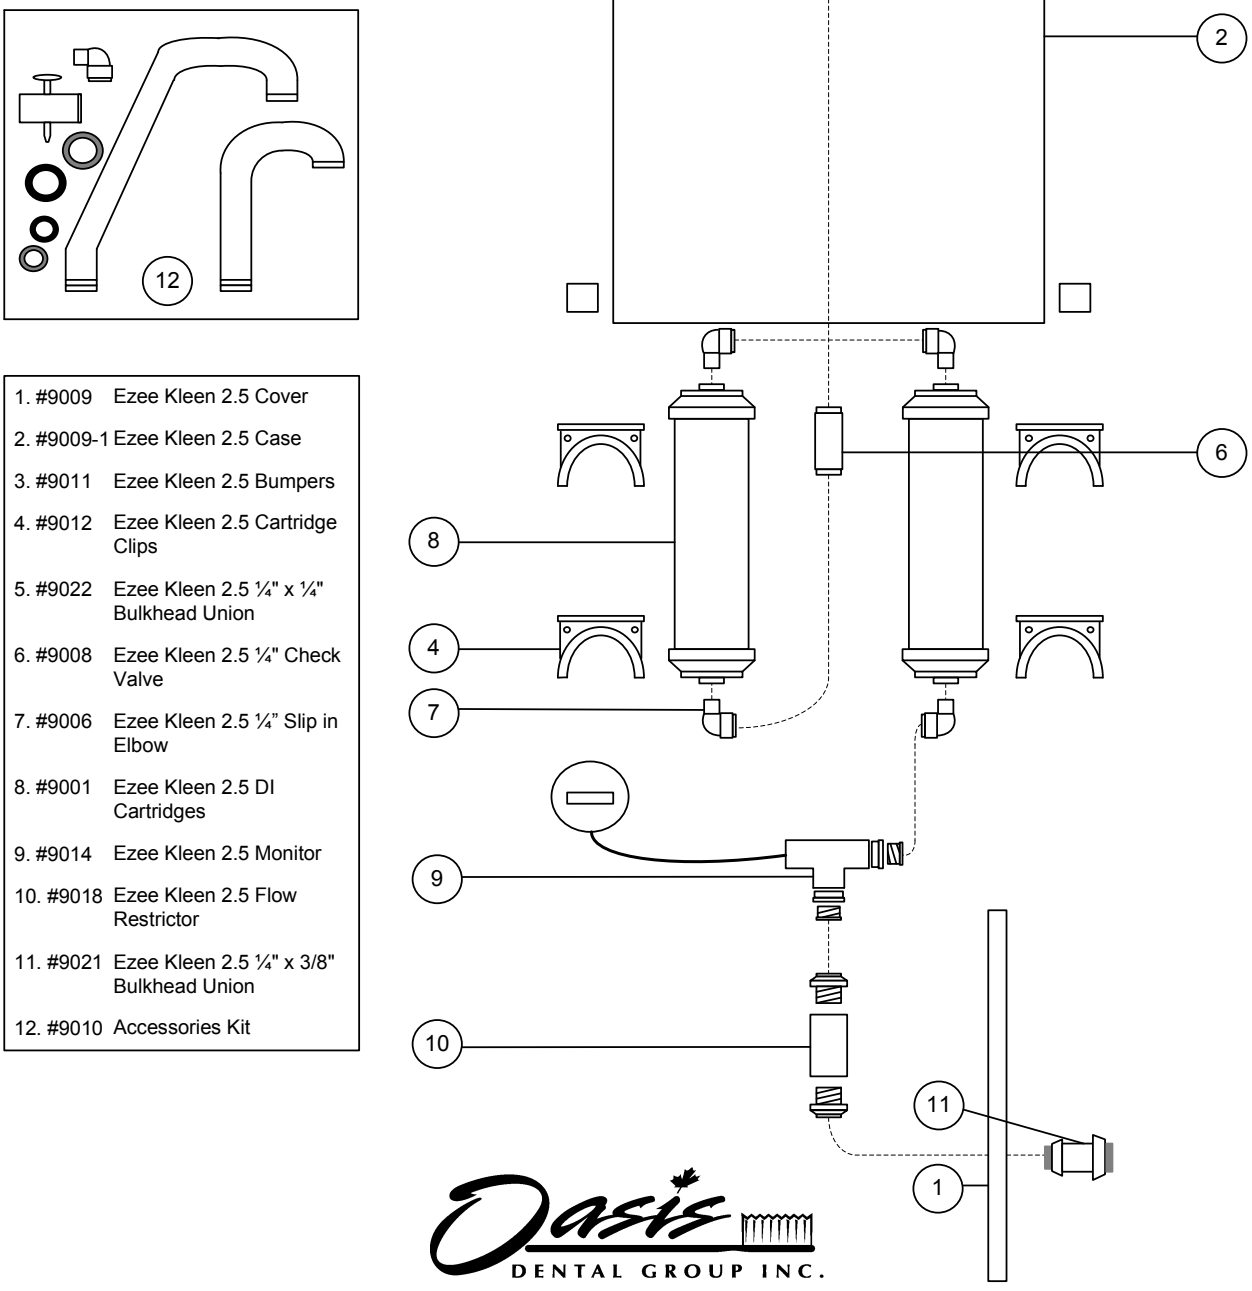

1.	#9009	Ezee Kleen 2.5 Cover
2.	#9009-1	Ezee Kleen 2.5 Case
3.	#9011	Ezee Kleen 2.5 Bumpers
4.	#9012	Ezee Kleen 2.5 Cartridge Clips
5.	#9022	Ezee Kleen 2.5 ¼" x ¼" Bulkhead Union
6.	#9008	Ezee Kleen 2.5 ¼" Check Valve
7.	#9006	Ezee Kleen 2.5 ¼" Slip in Elbow
8.	#9001	Ezee Kleen 2.5 DI Cartridges
9.	#9014	Ezee Kleen 2.5 Monitor
10.	#9018	Ezee Kleen 2.5 Flow Restrictor
11.	#9021	Ezee Kleen 2.5 ¼" x 3/8" Bulkhead Union
12.	#9010	Accessories Kit

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

GUARANTEE/WARRANTY

The **EZEEKLEEN 2.5** is guaranteed to produce the quality of water necessary to comply with all autoclave/steam sterilizer manufacturer's TDS (total dissolved solids) requirements when used in accordance with manufacturer's directions. This unit is intended to be used with source water meeting USA EPA National Drinking Water Regulations or Canadian Drinking Water Guidelines. Do not supply the **EZEEKLEEN 2.5** with water that is microbiologically unsafe or of unknown quality without adequate disinfection before or after the unit. Liability is limited to autoclave/sterilizer boiler repair or replacement while under manufacturer's warrantee upon given proof manufacturer's TDS requirements have not been met when the **EZEEKLEEN 2.5** has been used in accordance with manufacturer's (Oasis) directions.

For a period of one year, Oasis Dental Group Inc. guarantees the **EZEEKLEEN 2.5** to be free of defects due to workmanship including all components (with the exception of the Deionization cartridge) when delivered to the customer in new, unused condition by an acknowledged dealer of Oasis Dental Group Inc. products.

In the event of failure due to such defects, within this period of time, the exclusive remedies shall be repair or replacement, at Oasis Dental Group Inc.'s option and without charge, of any defective part(s) provided to Oasis Dental Group Inc. in writing within thirty (30) days of the date of such failure and further provided that the defective part(s) are returned to Oasis Dental Group Inc. freight prepaid.

Any express warranty not provided here on, or any implied warranty or representation as to the performance which may arise by implication not in this provision for the **EZEEKLEEN 2.5** is excluded and disclaimed by Oasis Dental Group Inc.

Warranty Certificate

Keep this and your original invoice of purchase in your permanent records for proof of warranty.

Name: _____

Address: _____

City: _____ State/Province: _____ Zip/Postal: _____

Phone Number: ( ) _____

Date of Purchase: Mo: _____ Day: _____ Year: _____

Dealer's Name: _____ City: _____

Oasis DENTAL GROUP INC.

16147 - 8A Avenue, Surrey, BC, V4A 8W8 ● Ph: (800) 338-6693 ● (604) 538-1285 ● Fax: (604) 538 - 1295

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca

© 2009-2012 Oasis Dental Group Inc.™
www.oasisdentalgroup.ca